PHILIPS COMPONENTS

DATA SHEET

Camera Tubes

XQ1073X

25.4 mm (1 inch) diameter Plumbicon® television camera tubes with high resolution lead-oxide photoconductive target, exclusively for use with X-ray image intensifiers with P20 output phosphor in medical equipment.

QUICK REFERENCE DATA

Diameter	25.4 mm (1 in)	
Length	approx. 162 mm	
Focusing	magnetic	
Deflection	magnetic	
Useful target area, circle diameter	15 mm	
Spectral response	see Fig. 3	
Sensitivity with P20 light source	typ. 500 μA/lmF	
Resolution	typ. 55%	
Heater	6.3 V, 95 mA	

XQ1073X

OPTICAL DATA

Dimensions of quality area on photoconductive target circle, dia 15 mm.

Orientation of image on target

For correct orientation of the image on the target the vertical scan should be essentially parallel to the plane passing through the tube axis and the mark on the tube base.

Faceplate

thickness $1.2 \pm 0.1 \text{ mm}$ refractive index n=1.49

ACCESSORIES

Socket type 56098

Deflection and focusing coil unit type AT1116S

ELECTRICAL DATA

Deflection magnetic

Focusing magnetic

Heating

Indirect by a.c. or d.c.

 $\begin{array}{lll} \mbox{Heater voltage} & \mbox{$V_{\rm f}$} & \mbox{6.3 V} \pm 5\% \\ \mbox{Heater current, at Vf} = 6.3 \mbox{ V} & \mbox{$I_{\rm f}$} & \mbox{nom 95 mA} \\ \end{array}$

The heater voltage must not exceed 9.5 V r.m.s. For optimum performance stabilization of the heater voltage is recommended.

Capacitance

Signal electrode to all C_{as} 3 to 5 pF

This capacitance, which is effectively the output impedance, increases when the tube is inserted in the coil unit.

Camera Tubes XQ1073X

LIMITING VALUES (Absolute maximum rating system)

All voltages are referred to the cathode, unless otherwise stated.				notes
Signal electrode voltage	V_{as}	max.	50 V	
Grid 4 voltage (mesh)	V_{g4}	max.	1100 V	
Grid 3 voltage	V_{g3}	max.	800 V	
Voltage between grid 4 and grid 3	$V_{\text{g4/g3}}$	max.	450 V	
Grid 2 voltage	V_{g2}	max.	350 V	
Grid 2 dissipation	\mathbf{W}_{g2}	max.	1W	
Grid 1 voltage, positive	V_{gl}	max.	0V	
Grid 1 voltage, negative	$-V_{g1}$	max.	125V	
Cathode to heater voltage, positive peak	$V_{\mathtt{kfp}}$	max.	125V	
Cathode to heater voltage, negative peak	$-V_{ ext{kfp}}$	max.	50 V	
Cathode heating time before drawing cathode current	\mathbf{t}_{h}	min.	1 min	
External resistance between cathode and heater at $V_{\rm kfp} > 10 \ V$	$R_{ t kf}$	min.	$2~\mathrm{k}\Omega$	
Ambient temperature, storage and operation	T_{amb}	max. min.	50°C -30°C	
Faceplate temperature, storage and operation	T	max. min.	50°C -30°C	1
Faceplate illuminance	E	max.	100 lx	2

OPERATING CONDITIONS AND PERFORMANCE

notes

Philips Components Slatersville, RI August 1997

Conditions		3
For a scanned circular area with a diameter of 15mm		
Cathode voltage	$V_{\mathtt{k}}$	0 V
Signal electrode voltage	$ m V_{as}$	45 V
Beam current	${ m I_b}$	4
Grid 4 voltage	$ m V_{g4}$	960 V
Grid 3 voltage	$ m V_{g3}$	600 V
Grid 2 voltage	$ m V_{g2}$	300 V
Grid 1 voltage	$ m V_{g1}$	4
Blanking voltage on grid 1, peak to peak	$V_{\tt gl\ p-p}$	50±10V
Faceplate illuminance (P20 light source)	Е	approx.1 lx
Faceplate temperature	T	20 to 45 °C
Electron Gun Characteristics		
Cutoff Grid 1 voltage for cut-off at $V_{g2} = 300V$ without blanking	$V_{ t gl}$	-35 to -100 V
Blanking voltage, peak to peak at $V_{\rm g2,4} = 300V$ on grid 1 on cathode	$\begin{matrix}V_{\texttt{gl} \ \texttt{p-p}}\\V_{kp-p}\end{matrix}$	50±10 V 25V
Grid 2 current at normally required beam currents	Ig2	≤ 0.5 mA
Performance Dark current	$\mathbf{I}_{\mathtt{d}}$	notes < 3 nA
Philips Components Slatersville, RI August 1997	Н	

XQ1073X

Camera Tubes	XQ1073X		
Sensitivity at colour temperature of 2856K	min. 400	typ. 485μA/Im	
Sensitivity with P20 light source	min. 90	typ. 115μA/ImF 5	
Peak signal current with E=1 lx (P20)	min. 160	typ. 195 nA 6	
Gamma of transfer characteristic		0.95 ± 0.05	
Spectral response:		see Fig. 3	
Resolution		7	
Modulation depth i.e. uncompensated amplitude response at 20.3 lp/mm (scanned area 9.6 mm x 12.8 mm) at the center of the picture (5 Mhz, 400 TV lines), BG 18 filter		typ 55%	
Modulation transfer characteristic		see Fig. 4	
Decay lag, P20 light source, measured with a signal current of 200 nA, beam adjusted for correct stabilization after the target has been illuminated for at least 5 s.			
Residual signal after dark pulse of 50 ms	max. 26%	typ. 22%	
Residual signal after dark pulse of 60 ms	max. 24%	typ. 20%	
Residual signal after dark pulse of 200 ms	max. 12%	typ. 8%	

NOTES




XQ1073X


- 1. The tube can withstand short excursions up to 70 °C without any damage or irreversible degradation in performance.
- 2. For short intervals. During storage the tube face shall be covered with the plastic hood provided; when the camera is idle the lens shall be capped, in stand-by also the beam will be cut-off.
- 3. The operating conditions and performance data quoted, relate to operation of the tube in coil units AT1116S. See relevant data of deflection/focusing assemblies. Scanning amplitude should be adjusted such that the useful target area of 15 mm is displayed on a standard monitor as a circular area with a diameter equal to the raster height.
- 4. The beam current I_b as obtained by adjusting the control grid voltage (grid 1) is set to max. 400 nA. Ib is not the total current available in the scanning beam, but is defined as the maximum amount of signal current I_s , that can be obtained with this beam. See note 6.
- 5. Measuring conditions: illuminance level 4.54 lx at a color temperature of 2856K and a filter Schott VG9 inserted in the light path.
- 6. The peak signal currents are measured on a waveform oscilloscope and with a uniform illumination on the 18 mm ϕ target area. When measured with an integrating instrument connected in the signal-electrode lead the average signal currents will be smaller:
 - a) By a factor α ($\alpha = \underline{100}$ - β), β being the total blanking time in %; for the CCIR system α 100

amounts to 0.75; for the EIA system α amounts to 0.83.

- b) By a factor δ , δ being the ratio of the active target area (circle with: 15 mm ϕ) to the area which would correspond with the adjusted scanning amplitude (15 mm x 20 mm). This ratio amounts to $\delta = 0.59$. The total ratio of integrated signal current, $I_{\rm s}$, to the peak signal current, $I_{\rm sp}$, amount to α x $\delta = 0.44$ for the CCIR system and 0.49 for EIA system.
- 7. As measured with a 50 mm Leitz Summicron lens having a sine response of approximately 85 % at 400 TV lines at f: 5.6. The published 55% typ. is uncorrected. Tube resolution is higher. Measured with 100 nA signal current and a beam current just sufficient to stabilize a signal current of 400 nA. The horizontal amplitude response can be raised by means of suitable correction circuits, which affect neither the vertical resolution nor the limiting resolution.

Diagrams








Fig. 4 Typical square-wave response curve.

Mechanical Data

Mounting Position: any Mass: approx. 60 g

Philips Components Slatersville, RI August 1997

-7-

Base: IEC 67-I-33a (JEDEC E8-11)

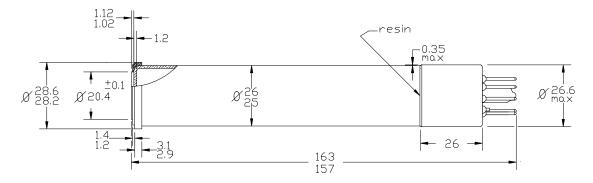


Figure 1.




Fig. 2a.





Fig 2b.



XQ1073X

Philips Camera Tubes Sales Offices

Philips Components Att: Kent Holston 4546 B10 El Camino Real #189

Los Altos, CA 94022 Tel: (650) 960-3893 Fax: (650) 960-3892

Philips Components Att: Mark Reinhardt

123 Nashua Road, Suite 244 Londonderry, NH 03053 Tel: (603) 425-7440 Fax: (603) 425-7416 Philips Components 100 Providence Pike Slatersville, RI 02876-2078

Tel: (401) 762-3800 Fax: (401) 767-4493

For Complimentary Literature, Call our Literature Center at 1-800-447-3762