
PHILIPS COMPONENTS

DATA SHEET

25.4 mm (1 inch) diameter Plumbicon® television camera tube designed specifically for high resolution fluoroscopy and digital imaging applications where both quantum noise and subtraction characteristics are required.

The XQ2182 series comprises the following versions:

- XQ2182/02X Rear loading, with target centering ring and BG18 anti-halation glass disk.
- XQ2182/03X Front loading, with metal ring and BG18 anti-halation glass disk.

Special features are:

- Ultra high resolution photoconductive target optimized for P20 phosphor.
- Variable lag using rear light bias.
- Diode Gun for high beam reserve and increased resolution.
- BG18 anti-halation disc for improved contrast.

QUICK REFERENCE DATA

“Diode” electron gun

Diameter	25.4 mm (1 in)
Length	approx. 170 mm
Focusing	magnetic
Deflection	magnetic
Useful target area, circle diameter	16.2 mm
Spectral response	See Fig. 3
XQ2182/02X	typ. 465 μ A/lmF
XQ2182/03X	typ. 465 μ A/lmF
Resolution	typ. 60%
Heater	6.3 V, 190 mA

®Registered Trade Mark for television camera tube

OPTICAL DATA

Dimensions of quality area on photoconductive target circle, dia 16.2 mm.

Orientation of image on target

For correct orientation of the image on the target the vertical scan should be essentially parallel to the plane passing through the tube axis and the mark on the tube base.

Faceplate

thickness	1.2 mm
refractive index	1.49

BG18 anti-halation glass disc (XQ2182/03X, XQ2182/02X)

thickness	1.07 mm
refractive index	1.54

ACCESSORIES

Socket	type 56605
--------	------------

Deflection and focusing coil unit,

XQ2182/02X	AT1126/03S
XQ2182/03X	AT1116S

ELECTRICAL DATA

Deflection	magnetic
------------	----------

Focusing	magnetic
----------	----------

Heating

Indirect by a.c. or d.c.

Heater voltage	V_f	$6.3 \text{ V} \pm 5\%$
----------------	-------	-------------------------

Heater current, at $V_f = 6.3 \text{ V}$	I_f	190 mA
--	-------	--------

The heater voltage must not exceed 9.5 V r.m.s. For optimum performance stabilization of the heater voltage is recommended.

Capacitance

Signal electrode to all

XQ2182/02X	2.5 to 4 pF
------------	-------------

XQ2182/03X	3 to 5 pF
------------	-----------

These capacitances, which are effectively the output impedances, increase when the tubes are inserted in the coil unit.

LIMITING VALUES (Absolute maximum rating system)

All voltages are referred to the cathode, unless otherwise stated.

notes

Signal electrode voltage	V_{as}	max.	50 V	
Grid 4 voltage (mesh)	V_{g4}	max.	1100 V	
Grid 3 voltage	V_{g3}	max.	800 V	
Voltage between grid 4 and grid 3	$V_{g4/g3}$	max.	450 V	
Grid 2 voltage	V_{g2}	max.	350 V	
Grid 1 voltage, positive	V_{g1}	max.	20 V	1
Grid 1 voltage, negative	$-V_{g1}$	max.	200 V	
Grid 1 current (\approx cathode current)	I_{g1}	max.	10 mA	3
Cathode to heater voltage, positive peak	V_{kfp}	max.	50 V	
Cathode to heater voltage, negative peak	$-V_{kfp}$	max.	125 V	
Cathode heating time before drawing cathode current	t_h	min.	1min	
External resistance between cathode and heater at $V_{kfp} > 10$ V	R_{kf}	min.	2 k Ω	
Ambient temperature, storage and operation	T_{amb}	max. min.	50 °C -30°C	
Faceplate temperature, storage and operation	T	max. min.	50 °C -30°C	4
Faceplate illuminance	E	max.	500 lx	5

OPERATING CONDITIONS AND PERFORMANCE			notes
Conditions			6
Cathode voltage	V_k	0 V	
Signal electrode voltage	V_{as}	45 V	
Beam current	I_b		2,7,8
Grid 4 voltage	V_{g4}	960 V	9
Grid 3 voltage	V_{g3}	600 V	9
Grid 2 voltage	V_{g2}	300 V	
Grid 1 voltage	V_{g1}	0 to 20V	
Blanking voltage on grid 1, peak to peak	$V_{g1 \text{ p-p}}$	30 V	
Focusing coil current			6
Deflection and alignment currents			6
Faceplate illuminance (P20 light source)	E	0 to 10 lx	
Faceplate temperature	T	20 to 40°C	
Electron Gun Characteristics			
Grid 1 voltage for cut-off at $V_{g2} = 300V$	V_{g1}	-10 to 0V	
Grid 1 voltage for normal beam setting	V_{g1w}	≤ 20 V	
Grid 1 current at normally required beam currents	I_{g1}	≤ 5 mA	
Grid 2 current at normally required beam currents	I_{g2}	$\leq 0,1$ mA	
Blanking voltage, peak to peak, with respect to V_{g1w}	$V_{g1 \text{ p-p}}$	30 V	
Performance			
Dark current	$I_d <$	2 nA	
Sensitivity at colour temperature of 2856K			10
XQ2182/02X	min. 380	typ. 465 $\mu A/lm$	
XQ2182/03X	min. 380	typ. 465 $\mu A/lm$	
Sensitivity with P20 light source			
XQ2182/02X	min. 80	typ. 110 $\mu A/lmF$	
XQ2182/03X	min. 80	typ. 110 $\mu A/lmF$	
Peak signal current with E=1 lx (P20)			11
XQ2182/02X	I_{sp} min. 175	typ. 215 nA	
XQ2182/03X	I_{sp} min. 175	typ. 215 nA	
Peak to current (16.2 mm dia scanning)		2000 nA	7

Gamma of transfer characteristic	0.95 \pm 0.05	notes
Philips Components	H	
Slatersville, RI		
August 1997		

Spectral response:	see Fig. 3			
Resolution				12
Modulation depth i.e. uncompensated amplitude response at 20.3 lp/mm (scanned area 9.6 x 12.8 mm) at the centre of the picture (5 Mhz, 400 TV lines)	min. 65%	typ. 75%		
Modulation depth at 12 lp/mm (scanned area 16.2mm diameter) at the centre of the picture (5MHz, 400 TV lines)	min. 80%	typ. 90%		
Modulation transfer characteristic	see Fig. 4			
Residual signal after dark pulse of 50 ms	min. 16%	typ. 20%	max. 25%	13,14
Residual signal after dark pulse of 200 ms		typ. 4.5%	max. 7%	

NOTES

1. The “Diode” gun operates with a positive grid 1 voltage, hence draws some grid current. The grid 1 voltage (d.c.) must be adjusted for correct beam current as described in note 8.

2. “Diode” gun is a triode gun operating in a diode mode, providing a very high beam reserve.

Continuous operation with a high beam setting is to be avoided since this will shorten tube life. High I_b settings should be used under high light intensity conditions only. All other modes of operation should be normal I_b settings or have then cut off.

3. A current limiter must be incorporated to limit total cathode current to 10 mA maximum.
4. The tube can withstand short excursions up to 70 °C without any damage or irreversible degradation in performance.
5. For short intervals. During storage the tube face shall be covered with the plastic hood provided; when the camera is idle the lens shall be capped, in stand-by also the beam will be cut-off.
6. The operating conditions and performance data quoted, relate to operation of the tube in coil units AT1116 or AT1126. See relevant data of deflection/focusing assemblies.
Scanning amplitude should be adjusted such that the useful target area of 16.2 mm dia. is displayed on a standard monitor as a circular area with a diameter equal to the raster height.
7. The maximum peak signal which can be handled is 3 μ A. Video amplifiers should be designed to accommodate this.

8. The beam current I_b as obtained by adjusting the control grid voltage (grid 1) is set at 400 nA. I_b is not the total current available in the scanning beam, but is defined as the maximum amount of signal current I_s , that can be obtained with this beam.

In the performance figures, e.g. for resolution and lag, the signal current and beam current conditions are given, e.g. as $I_s/I_b = 20/300$ nA. This means: with a signal current of 20 nA and a beam setting which just allows a signal current of 300 nA.

N.B. The signal currents are measured with an integrating instrument connected in the signal electrode lead and a uniform illumination of the scanned area. See note 11.

9. The optimum voltage ratio V_{g4}/V_{g3} to minimize beam landing error (preferable ≤ 1 V) depends on the type of coil unit used. For types AT1116 and AT1126 a ratio of 1.6 is recommended. Grid 4 (mesh) should under no circumstances be allowed to operate at a voltage below that of grid 3 as that might damage the target.
10. Measuring conditions: illuminance level 4.54 lx at a colour temperature of 2856K and filters. Schott VG9 and Calflex B1/K1 inserted in the light path.

Notes (continued)

11. The peak signal currents are measured on a waveform oscilloscope and with a uniform illumination on the 16.2 mm ϕ target area.
When measured with an integrating instrument connected in the signal-electrode lead the average signal currents will be smaller:
- a) By a factor α ($\alpha = \frac{100-\beta}{100}$), β being the total blanking time in %; for the CCIR system α amounts to 0.75; for the NTSC system α amounts to 0.83.
 - b) By a factor δ , δ being the ratio of the active target area (circle with: 16.2 mm ϕ) to the area which would correspond with the adjusted scanning amplitude (16.2 mm x 21.6 mm) this ratio amounts to $\delta = 0.59$.
The total ratio of integrated signal current, I_s , to the peak signal current, I_{sp} , amount to $\alpha \times \delta = 0.44$ for the CCIR system and 0.49 for NTSC system.
12. As measured with a 50 mm Leitz Summicron lens having a sine response of approximately 85 % at 400 TV lines at $f : 5.6$. The published 75% typ. is uncorrected. Tube resolution is higher. Measured with 200 nA signal current and a beam current just sufficient to stabilize a signal current of 400 nA. The horizontal amplitude response can be raised by means of suitable correction circuits, which affect neither the vertical resolution nor the limiting resolution.
13. Measured with a 20 nA signal current and a beam current just sufficient to stabilize a signal current of 30 nA.
14. Decay lag. After a minimum of 5 s of illumination of the target. Values shown relating to decay lag represent the residual signal currents in percentages of the original signal current as a function of time, after the illumination has been removed.

Diagrams

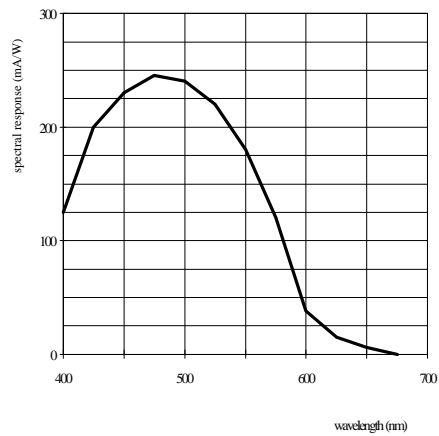


Fig. 3 Typical spectral response curve.


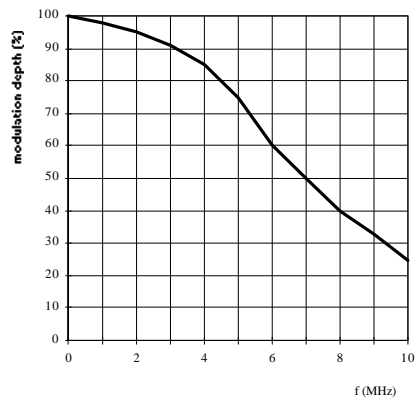


Fig. 4 Typical square-wave response curve.

Mechanical Data

Rear loading tubes XQ2182/02X

Mechanical Data

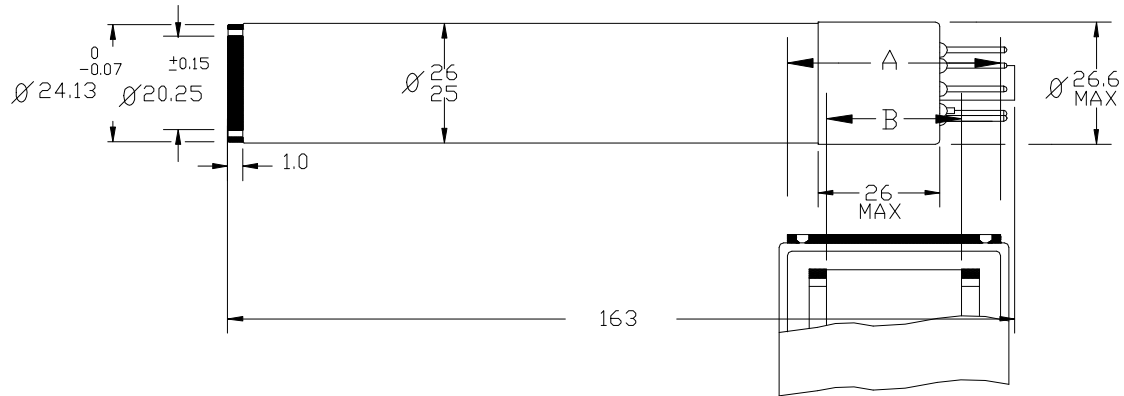

Front loading tubes XQ2182/03X

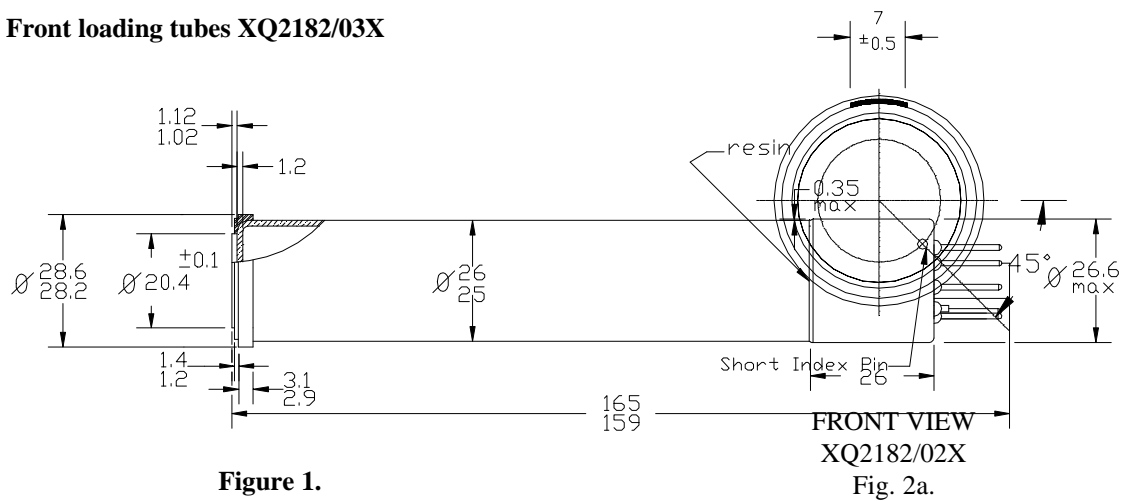


Figure 1.

Fig. 2a.

(1) The distance between the geometrical centers of diameter A of the reference ring and diameter B of the mesh electrode ring is $< 100 \mu\text{m}$.

Mounting position: any

Mass: $\approx 70\text{g}$

Base: IEC 67-I-33a (JEDEC E8-11)

Philips Components
Slatersville, RI
August 1997

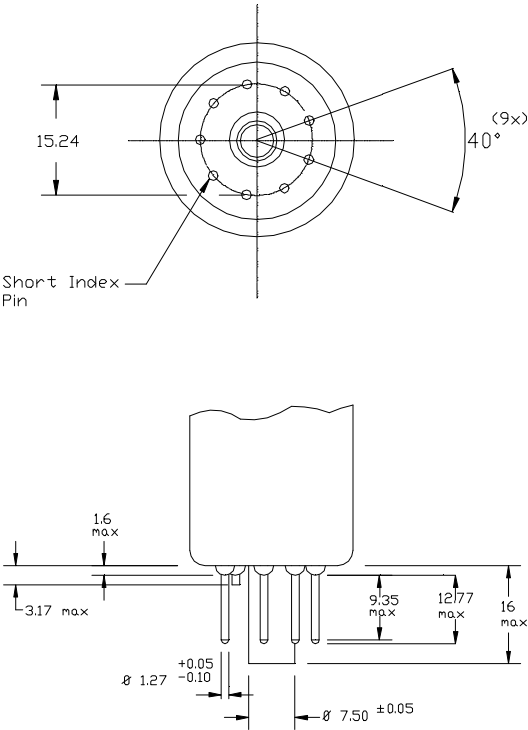


Fig. 2b.

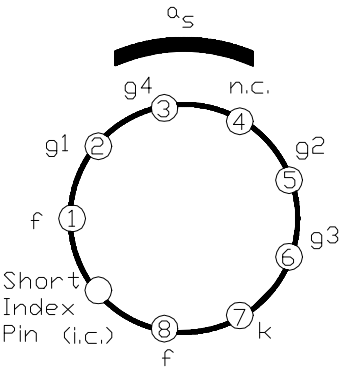


Fig. 2c.

Philips Camera Tubes Sales Offices

Philips Components
Att: Kent Holston
4546 B10 El Camino Real #189
Los Altos, CA 94022
Tel: (650) 960-3893
Fax: (650) 960-3892

Philips Components
Att: Mark Reinhardt
123 Nashua Road, Suite 244
Londonderry, NH 03053
Tel: (603) 425-7440
Fax: (603) 425-7416

Philips Components

100 Providence Pike
Slatersville, RI 02876-2078
Tel: (401) 762-3800
Fax: (401) 767-4493

For Complimentary Literature, Call our Literature Center at 1-800-447-3762