

PHILIPS COMPONENTS

DATA SHEET

Camera Tubes

XQ5002

30mm/45mm diameter, Plumbicon® television camera tube with very high resolution lead-oxide photoconductive target, exclusively intended for use with X-ray image intensifiers in medical equipment.

Special features are:

- Large scan area,
- Electrostatic deflection for improved corner resolution,
- New photoconductive target for increased resolution,
- “Diode” electron gun for high beam reserve, improved beam acceptance, low lag,
- Low output capacitance for high signal-to-noise ratio,
- Possibility of scan rotation,

QUICK REFERENCE DATA

“Diode” electron gun	notes 1,2
Diameter	47mm/30mm
Length	approx. 170mm
Focusing	magnetic
Deflection	electrostatic
Useful target area, circle diameter	26 mm
Spectral response	see Fig. 3
Sensitivity with P20 light source	typ. 115 $\mu\text{A}/\text{lmF}$
Resolution	typ. 95%
Heater	6.3 V, 190 mA

®Registered Trade Mark for television camera tube

Philips Components
Slatersville, RI
August 1997

OPTICAL DATA

notes

Dimensions of quality area of target, circle of 26mm diameter

3

Orientation of image on target

For correct orientation of the image on the target the vertical scan should be essentially parallel to the plane passing through the tube axis and the index pin.

Faceplate

thickness

3 mm

refractive index

n= 1.49

Anti halation glass disc

thickness

8 mm

refractive index

1.52 mm

ACCESSORIES

Socket

type: Novar 4 87 A01

Deflection and focusing coil unit

type: Cletronics #5134-02-2453

ELECTRICAL DATA

Deflection

electrostatic

Focusing

magnetic

Heating

Indirect by a.c. or d.c.

Heater voltage

 V_f 6.3 V \pm 5%Heater current, at $V_f = 6.3$ V I_f nom 190 mA

The heater voltage must not exceed 9.5 V r.m.s. For optimum performance stabilization of the heater voltage is recommended.

Capacitance

Signal electrode to all

 C_{as} 5 pF

This capacitance, which is effectively the output impedance, increases when the tube is inserted in the coil unit.

LIMITING VALUES (Absolute maximum rating system)

All voltages are referred to the cathode, unless otherwise stated.

notes

Signal electrode voltage	V_{as}	max.	50 V	
Grid 4 voltage (mesh)	V_{g4}	max.	1100 V	
Grid 3 voltage	V_{g3}	max.	1000 V	
Voltage between grid 4 and grid 3	$V_{g4/g3}$	max.	450 V	5
Grid 2 voltage	V_{g2}	max.	500 V	
Grid 1 voltage, positive	V_{g1}	max.	20V	
Grid 1 voltage, negative	$-V_{g1}$	max.	125V	
Grid 1 current (\approx cathode current)	I_{g1}	max.	10mA	4
Cathode heating time before drawing cathode current	th	min.	1 min.	

notes

Cathode to heater voltage, positive peak	V_{kfp}	max.	50V	
Cathode to heater voltage, negative peak	$-V_{kfp}$	max.	125 V	
External resistance between cathode and heater at $V_{kf} > 10V$	R_{kf}	min.	2 k Ω	
Ambient temperature, storage and operation	T_{amb}	max. min.	50°C 30°C	6
Faceplate temperature, storage and operation	T	max. min.	50°C -30°C	
Faceplate illuminance	E	max.	500 lx	

OPERATING CONDITIONS AND PERFORMANCE

High

Low

notes

Camera Tubes**XQ5002**

Conditions		Voltage t yp.	Voltage typ.	
Cathode voltage	V_k	0 V	0 V	
Signal electrode voltage	V_{as}	45 V	45 V	
Beam current	I_b			8, 9
Grid 4 voltage	V_{g4}	1000 V	550 V	5
Grid 3 voltage	V_{g3}	600 V	360 V	5
Grid 2 voltage	V_{g2}	360 V	360 V	
Grid 1 voltage	V_{g1}	0 to 20 V	0 to 20 V	
Blanking voltage on grid 1, peak to peak	V_{g1p-p}	25 V	25 V	
Focusing and deflection coil currents				10
Faceplate illuminance	E	0 to 10 lx	0 to 10 lx	
Faceplate temperature	T_{as}	20 to 40 °C	20 to 40 °C	
Deflection element voltage		600 V DC	330 V DC	
Deflection ramp voltage		400 V p-p	230 V p-p	
Focus coil operation		86mA @ 16 V	65 mA @ 12 V	

Electron Gun Characteristics**Cut-off**

Grid 1 voltage for cut-off at $V_{g2} = 300V$ without blanking	V_{g1}	-10 to 0 V	
Grid voltage for normal beam current	V_{g1w}	9 V	
Blanking voltage with respect to V_{g1w} , peak-to-peak, on grid 1 on cathode	$V_{g1 p-p}$ V_{kp-p}	25 V 25 V	
Grid 1 current at normally required beam currents	I_{g1}	≤ 5 mA	
Grid 2 current at normally required beam currents	I_{g2}	≤ 0.1 mA	

Performance

Dark current	I_d	< 3 nA	notes
--------------	-------	--------	-------

Camera Tubes

XQ5002

Sensitivity at colour temperature of 2856K	typ.	115 μ A/lmF	11
Sensitivity with P20 light source	typ.	350 μ A/lmF	
Peak signal current with E+1 lx (P20)	I _{sp} typ.	420 nA	12
Peak signal current (26 mm dia.)		3500 nA	
Spectral response:			
max. response at		\approx 500 nm	
cut -off at		850 to 950 nm	
response curves	see Fig. 2		
Gamma of transfer characteristic		0.95 \pm 0.05	

Resolution

Modulation depth i.e. uncompensated amplitude response at 400 TV lines at center of the picture
(At corners, resolution is 80% of center resolution)

	XQ5002V
Highlight signal current I _s	400 nA
Beam current I _b	800 nA
Modulation depth at 400 TV lines (5 Mhz in % typ.)	95
min.	90

		Notes
Limiting resolution	2500 TV lines	
Modulation transfer charactersitic		13
Lag (typical values)		8,14,15,16
Light source with a color temperrature of 2856 K Appropriate filter inserted in light path.		11

HIGH BEAM PERFORMANCE

Resolution

Corrected amplitude response at 400 TVL at center of picture.

(At corners, resolution is 80% of center resolution.)

for $I_b/I_s = 2400/400$ nA	min. 75%
	max. 80%
for $I_b/I_s = 2400/200$ nA	min. 65%
	max. 70%

Resolution

Corrected amplitude response at 1000 TVL at center of picture

(At corners, resolution is 80% of center resolution.)

for $I_b/I_s = 2400/400$ nA	min. 40%
	max. 50%

Diagrams

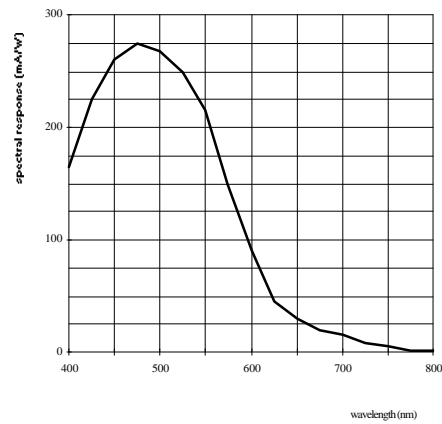


Fig. 3 Typical spectral response curve.

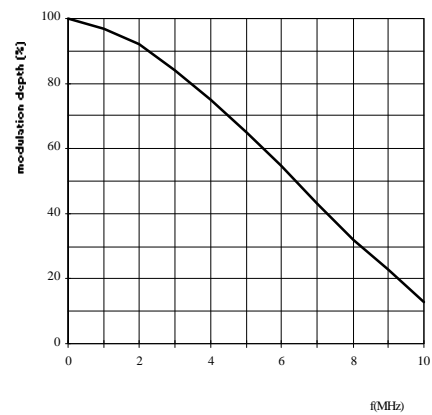


Fig. 4 Typical square-wave response curve.

NOTES

1. Diode gun is a triode gun operating in a diode mode, providing a very high beam reserve. Continuous operation with a high beam setting is to be avoided since this will shorten tube life. High I_b settings should be used under high light intensity conditions only, such as pulsed mode and rad mode. All other modes of operation should be normal I_b settings or have beam cut off.
2. The Diode gun requires a positive grid 1 voltage, and draws some grid current.
3. Underscanning of the specified target area (26mm diam.), or failure of scanning, should be avoided since damage to the target may occur. Cathode blanking should be used to provide a circular image. Video blanking could cause beam to scan mesh ring, with possible consequent degradation of tube life.
4. A current limiter must be incorporated to limit total cathode current to 10 mA maximum. Camera design should allow for 10 mA operation.
5. The optimum voltage ratio V_{g4}/V_{g3} to minimize beam landing errors (preferable <1 V) depends on the type of coil used. For type AT1107/01, a ratio of 1.6 is recommended. Under no circumstances should grid 4 (mesh) be allowed to operate at a voltage below that of grid 3 as this may damage the target.
6. The tube can withstand short excursions to 70 °C without any damage or irreversible degradation in performance.
7. This rating is for short intervals only. During storage the tube must be covered (a plastic hood is provided for this purpose) and when the camera is idle the lens must be capped. **If camera is in stand-by operation, the lens must be capped and the beams turned off.**
8. The beam current I_b , as obtained by adjusting the control grid voltage (grid 1) is set at 800 nA. I_b is not the total current available in the scanning beam, but is defined as the maximum amount of signal current I_s , with this particular beam setting. In the performance figures, e.g. for resolution and lag, the signal current and beam current conditions are given, e.g. as $I_s / I_b = 400/800$ nA. This means: with signal current of 400 nA and a beam setting which just allows a signal current of 800 nA.

N.B. The signal currents are measured with an integrating instrument connected in the signal electrode lead and a uniform illumination of the scanned area. The peak signal currents as measured on a waveform oscilloscope will be a factor α larger. See note 12.
9. The maximum peak signal which the XQ5002/A can handle is 4 μ A. Video amplifiers should be designed to accommodate this.
10. See published data of deflection/focusing assemblies. The direction of the current through the focusing coil should be chosen such that a north-seeking pole will be attracted at the faceplate end of the coil.
11. Measuring conditions: Illuminance level 3.1 lx at a colour temperature of 2856K. Filters Schott VG9(1mm) and Calflex B1/K1 inserted in the light path. For transmission curves see General Section.

Notes: continued

12. The peak signal currents are measured on a waveform oscilloscope and with a uniform illumination on the 26 mm ϕ target area. When measured with an integrating instrument connected in the signal-electrode lead the average signal currents will be smaller:

- a) By a factor α ($\alpha = \frac{100-\beta}{100}$), β being the total blanking time in %; for the CCIR system α amounts to 0.75; for the EIA system α amounts to 0.83.
- b) By a factor δ , δ being the ratio of the active target area (circle with: 26 mm ϕ) to the area which would correspond with the adjusted scanning amplitude (26 mm x 34.6 mm) this ratio amounts to $\delta = 0.59$.

The total ratio of integrated signal current, I_s , to the peak signal current, I_{sp} , amount to $\alpha \times \delta = .44$ for the CCIR system and 0.49 for EIA system.

13. As measured with a 50 mm Leitz Summicron lens having a sine response of approximately 96 % at 8 Ip/mm (400 TV lines at 26 mm dia.) at $f : 5.6$. The published 95% typ. is uncorrected. Tube resolution is higher.

The horizontal amplitude response can be raised by means of suitable correction circuits, which affect neither the vertical resolution nor the limiting resolution.

14. Measured with a 100 nA signal current and a beam current just sufficient to stabilize a signal current of 800 nA.
15. *Build-up lag.* After 10 seconds of complete darkness. Values and curves shown relating to build-up lag represent the typical percentages of the ultimate signal obtained as a function of time, after the illumination has been applied.
16. *Decay lag.* After a minimum of 5 seconds of illumination of the target. Values and curves shown relating to decay lag represent the residual signal currents in percentages of the original signal current as a function of time, after the illumination has been removed.

Mechanical Data

Philips Components
Slatersville, RI
August 1997

Philips Camera Tubes Sales Offices

Philips Components
Att: Kent Holston
4546 B10 El Camino Real #189
Los Altos, CA 94022
Tel: (650) 960-3893
Fax: (650) 960-3892

Philips Components
Att: Mark Reinhardt
123 Nashua Road, Suite 244
Londonderry, NH 03053
Tel: (603) 425-7440
Fax: (603) 425-7416

Philips Components

100 Providence Pike
Slatersville, RI 02876-2078
Tel: (401) 762-3800
Fax: (401) 767-4493

For Complimentary Literature, Call our Literature Center at 1-800-447-3762